

KEY NOTES

1. MOUNT A5145, HOOK, AT 1372 [4'-6"] AFF.
2. INCREASE THIS DIMENSION AS NEEDED TO COMPLY WITH ADA IF THE DOOR HAS A CLOSER OR IF 610 [2'-0"] CLEARANCE IS NOT AVAILABLE AT THE STRIKE SIDE OF THE DOOR.
3. COORDINATE LOCATION OF M1620, PATIENT CHART HOLDER, AND ROOM SIGNAGE.
4. LENGTH OF E1500, WALL MOUNTED RAIL, TO BE DETERMINED BY MANUFACTURER/INSTALLER.
5. MOUNT A5145, HOOK, AT 1219 [4'-0"] AFF. PROVIDE 2-A5145'S FOR NAVY PROJECTS ONLY. MOUNT 1-A5145 AT 1219 [4'-0"] AFF AND 1-A5145 AT 1524 [5'-0"] AFF.
6. P3200, ELECTRONIC LAVATORY, MAY BE USED INSTEAD OF P3100, LAVATORY. FOR THE P3200 PROVIDE EITHER BATTERY POWER OR HARD WIRED CONNECTION.

OUTPATIENT EMG ROOM (PTEM1)

3.12.02

ORTHOPEDICS/PODIATRY


0 1000 2000

FLOOR/EQUIPMENT PLAN 11.15 NSM (120 NSF)



DATE: 01/28/2002

1:50 SCALE (MILLIMETERS)

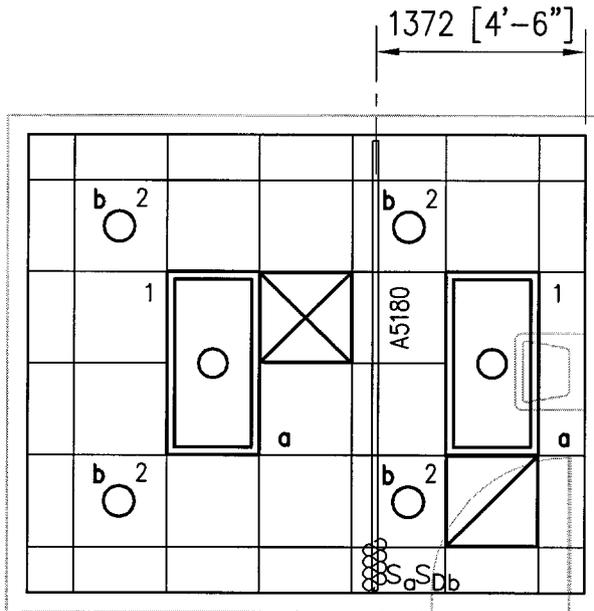

KEY NOTES

1. PROVIDE SHIELDED LENS TO PREVENT INTERERENCE WITH EMG EQUIPMENT.
2. PROVIDE INCANDESCENT LIGHTS.

OUTPATIENT EMG ROOM (PTEM1)

3.12.02

ORTHOPEDICS/PODIATRY


CEILING PLAN

DATE: 01/28/2002


0 1000 2000




1:50 SCALE (MILLIMETERS)

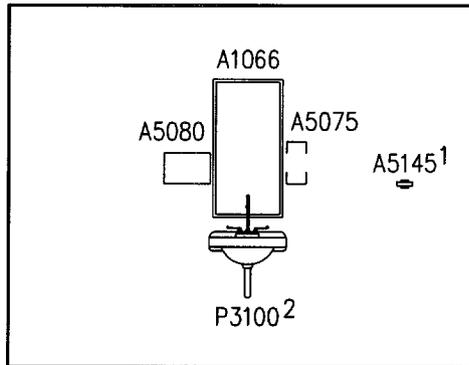


EAST

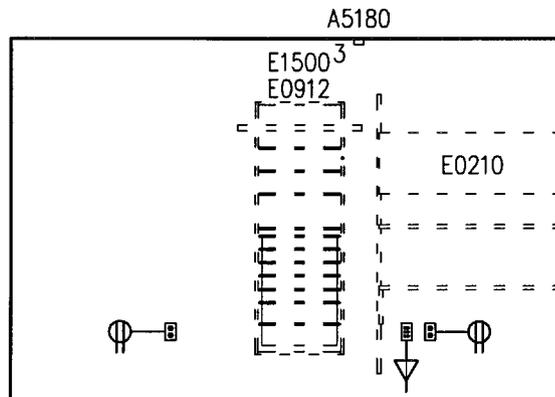

NORTH

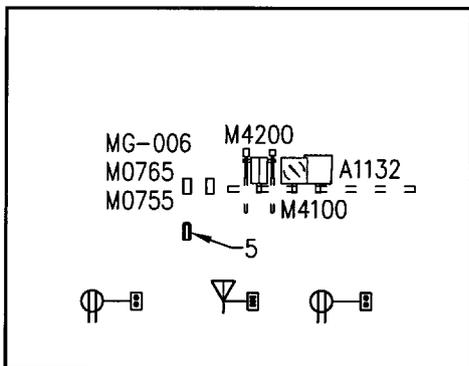

WEST

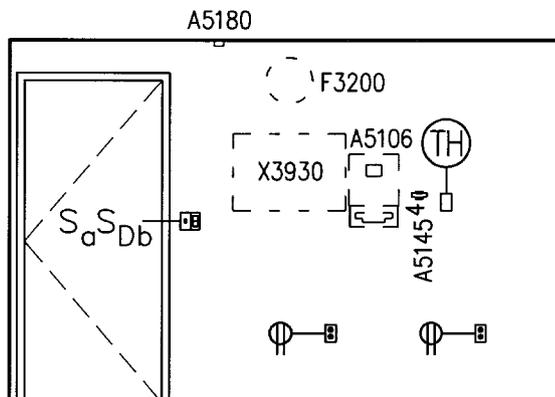

SOUTH

NOTES

1. SEE TYPICAL EQUIPMENT MOUNTING HEIGHTS BEGINNING ON SHEET 7.01.01.

KEY NOTES

1. MOUNT A5145, HOOK, AT 1219 [4'-0"] AFF. PROVIDE 2-A5145'S FOR NAVY PROJECTS ONLY. MOUNT 1-A5145 AT 1219 [4'-0"] AFF AND 1-A5145 AT 1524 [5'-0"] AFF.
2. P3200, ELECTRONIC LAVATORY, MAY BE USED INSTEAD OF P3100, LAVATORY. FOR THE P3200 PROVIDE EITHER BATTERY POWER OR HARD WIRED CONNECTION.
3. LENGTH OF E1500, WALL MOUNTED RAIL, TO BE DETERMINED BY MANUFACTURER/INSTALLER.
4. MOUNT A5145, HOOK, AT 1372 [4'-6"] AFF.
5. VACUUM SLIDE.

OUTPATIENT EMG ROOM (PTEM1)

3.12.02

ORTHOPEDICS/PODIATRY

ELEVATIONS

DATE: 01/28/2002

0 1000 2000



1:50 SCALE (MILLIMETERS)

Medical Equipment Room Guide Plates

3.12 Orthopedics/Podiatry

Plate Number 3.12.02
Room Name OUTPATIENT EMG ROOM
SEPS # PTEM1

| JSN | Nomenclature | Qty | Army | Navy | AF | Utilities | | | | | |
|-------|--|-----|------|------|-----|-----------|---|---|---|---|---|
| | | | Cat | Cat | Cat | 1 | 2 | 3 | 4 | 5 | 6 |
| A1066 | Mirror, Float Glass, With SS Frame, 36X18 | 1 | A | A | A | . | . | . | . | . | J |
| A1132 | Rail, Accessory Mounting, Length As Required | 1 | C | C | C | . | . | . | . | . | . |
| A5075 | Dispenser, Soap, Disposable | 1 | C | C | C | . | . | . | . | . | . |
| A5080 | Dispenser, Paper Towel, SS, Surface Mounted | 1 | A | A | A | . | . | . | . | . | J |
| A5106 | Waste Disposal Unit, Sharps w/Glove Dispenser | 1 | C | A | C | . | . | . | . | . | . |
| A5145 | Hook, Garment, Double, SS, Surface Mounted | 2 | A | A | A | . | . | . | . | . | J |
| A5180 | Track, Cubicle, Surface Mounted, With Curtain | 1 | A | A | A | . | . | . | . | . | J |
| E0210 | Worksurface, w/Overhead Cab, Wall Mtd, 48" W | 1 | C | C | C | . | A | . | . | . | J |
| E0912 | Locker, Supply, Med Surg, Wall Mtd, 23"W x 20"D | 1 | C | C | C | . | . | . | . | . | . |
| E1500 | Rail, MOD, W/MNTD, HX144XD | 1 | C | C | C | . | . | . | . | . | J |
| F0280 | Chair, Swivel, Low Back | 1 | C | C | C | . | . | . | . | . | . |
| F0340 | Stool, Self Adjusting | 1 | C | C | C | . | . | . | . | . | . |
| F0355 | Footstool, Straight | 1 | C | C | C | . | . | . | . | . | . |
| F2000 | Basket, Wastepaper, Round, Metal, 18 H x 16 Dia. | 2 | C | C | C | . | . | . | . | . | . |
| F3200 | Clock, Battery, 12" Diameter | 1 | C | C | C | . | . | . | . | . | . |
| M0755 | Flowmeter, Oxygen, Low Flow | 1 | C | C | C | . | . | A | . | . | . |
| M0765 | Regulator, Vacuum | 1 | C | C | C | . | . | B | . | . | . |
| M1620 | Holder, Chart, Patient, Wall or Door Mounted | 1 | A | A | A | . | . | . | . | . | . |
| M1800 | Computer, Microprocessing | 1 | C | C | C | . | A | . | . | . | . |
| M3070 | Hamper, Linen, Mobile, w/Lid | 1 | C | C | C | . | . | . | . | . | . |
| M3072 | Frame, Infectious Waste Bag w/Lid | 1 | C | C | C | . | . | . | . | . | . |
| M4100 | Sphygmomanometer, Aneroid, Wall Mounted | 1 | C | C | C | . | . | . | . | . | . |
| M4200 | Otoscope/Ophthalmoscope, Wall Mounted | 1 | C | C | C | . | A | . | . | . | . |
| M4655 | Stretcher, Mobile, CRS, 9 Position | 1 | C | C | C | . | . | . | . | . | . |
| M7725 | Electromyograph | 1 | C | C | C | . | A | . | . | . | . |
| M8120 | Therapy Unit, Hydroculator | 1 | C | C | C | . | A | . | . | . | . |
| P3100 | Lavatory, Vitreous China, Slab Type | 1 | A | A | A | D | . | . | . | . | . |
| X3930 | Illuminator, Film, Double, Wall Mounted, 20x29x6 | 1 | C | C | C | . | A | . | . | . | J |